



UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

APPLICATION NO.	FILING DATE	FIRST NAMED INVENTOR	ATTORNEY DOCKET NO.	CONFIRMATION NO.
10/614,549	07/03/2003	Charles R. Mooney	ECC-5527DIV	5851
<div>7590 Edwards Lifesciences LLC Law Dept. One Edwards Way Irvine, CA 92614</div>			<div>EXAMINER MENDEZ, MANUEL A</div>	
			<div>ART UNIT 3763</div>	<div>PAPER NUMBER</div>
			<div>MAIL DATE 12/03/2008</div>	<div>DELIVERY MODE PAPER</div>

Please find below and/or attached an Office communication concerning this application or proceeding.

The time period for reply, if any, is set in the attached communication.

Office Action Summary	Application No. 10/614,549	Applicant(s) MOONEY ET AL.	
	Examiner Manuel A. Mendez	Art Unit 3763	

-- The MAILING DATE of this communication appears on the cover sheet with the correspondence address --

Period for Reply

A SHORTENED STATUTORY PERIOD FOR REPLY IS SET TO EXPIRE 3 MONTH(S) OR THIRTY (30) DAYS, WHICHEVER IS LONGER, FROM THE MAILING DATE OF THIS COMMUNICATION.

- Extensions of time may be available under the provisions of 37 CFR 1.136(a). In no event, however, may a reply be timely filed after SIX (6) MONTHS from the mailing date of this communication.
- If NO period for reply is specified above, the maximum statutory period will apply and will expire SIX (6) MONTHS from the mailing date of this communication.
- Failure to reply within the set or extended period for reply will, by statute, cause the application to become ABANDONED (35 U.S.C. § 133). Any reply received by the Office later than three months after the mailing date of this communication, even if timely filed, may reduce any earned patent term adjustment. See 37 CFR 1.704(b).

Status

- 1) ☐ Responsive to communication(s) filed on ____.
- 2a) ☐ This action is **FINAL**. 2b) ☒ This action is non-final.
- 3) ☐ Since this application is in condition for allowance except for formal matters, prosecution as to the merits is closed in accordance with the practice under *Ex parte Quayle*, 1935 C.D. 11, 453 O.G. 213.

Disposition of Claims

- 4) ☒ Claim(s) 1-4 is/are pending in the application.
4a) Of the above claim(s) ____ is/are withdrawn from consideration.
- 5) ☐ Claim(s) ____ is/are allowed.
- 6) ☒ Claim(s) 1-4 is/are rejected.
- 7) ☐ Claim(s) ____ is/are objected to.
- 8) ☐ Claim(s) ____ are subject to restriction and/or election requirement.

Application Papers

- 9) ☐ The specification is objected to by the Examiner.
- 10) ☐ The drawing(s) filed on ____ is/are: a) ☐ accepted or b) ☐ objected to by the Examiner.
Applicant may not request that any objection to the drawing(s) be held in abeyance. See 37 CFR 1.85(a).
Replacement drawing sheet(s) including the correction is required if the drawing(s) is objected to. See 37 CFR 1.121(d).
- 11) ☐ The oath or declaration is objected to by the Examiner. Note the attached Office Action or form PTO-152.

Priority under 35 U.S.C. § 119

- 12) ☐ Acknowledgment is made of a claim for foreign priority under 35 U.S.C. § 119(a)-(d) or (f).
a) ☐ All b) ☐ Some * c) ☐ None of:
1. ☐ Certified copies of the priority documents have been received.
 2. ☐ Certified copies of the priority documents have been received in Application No. ____.
 3. ☐ Copies of the certified copies of the priority documents have been received in this National Stage application from the International Bureau (PCT Rule 17.2(a)).

* See the attached detailed Office action for a list of the certified copies not received.

Attachment(s)

- | | |
|---|---|
| 1) <input checked="" type="checkbox"/> Notice of References Cited (PTO-892) | 4) <input type="checkbox"/> Interview Summary (PTO-413)
Paper No(s)/Mail Date. ____. |
| 2) <input type="checkbox"/> Notice of Draftsperson's Patent Drawing Review (PTO-948) | 5) <input type="checkbox"/> Notice of Informal Patent Application |
| 3) <input checked="" type="checkbox"/> Information Disclosure Statement(s) (PTO/SB/08)
Paper No(s)/Mail Date <u>07/03/2003</u> . | 6) <input type="checkbox"/> Other: ____. |

DETAILED ACTION

Claim Rejections - 35 USC § 102

The following is a quotation of the appropriate paragraphs of 35 U.S.C. 102 that form the basis for the rejections under this section made in this Office action:

A person shall be entitled to a patent unless –

(b) the invention was patented or described in a printed publication in this or a foreign country or in public use or on sale in this country, more than one year prior to the date of application for patent in the United States.

(e) the invention was described in (1) an application for patent, published under section 122(b), by another filed in the United States before the invention by the applicant for patent or (2) a patent granted on an application for patent by another filed in the United States before the invention by the applicant for patent, except that an international application filed under the treaty defined in section 351(a) shall have the effects for purposes of this subsection of an application filed in the United States only if the international application designated the United States and was published under Article 21(2) of such treaty in the English language.

(e) the invention was described in a patent granted on an application for patent by another filed in the United States before the invention thereof by the applicant for patent, or on an international application by another who has fulfilled the requirements of paragraphs (1), (2), and (4) of section 371(c) of this title before the invention thereof by the applicant for patent.

The changes made to 35 U.S.C. 102(e) by the American Inventors Protection Act of 1999 (AIPA) and the Intellectual Property and High Technology Technical Amendments Act of 2002 do not apply when the reference is a U.S. patent resulting directly or indirectly from an international application filed before November 29, 2000. Therefore, the prior art date of the reference is determined under 35 U.S.C. 102(e) prior to the amendment by the AIPA (pre-AIPA 35 U.S.C. 102(e)).

Claims 1, 2, and 4 are rejected under 35 U.S.C. 102(b) as being anticipated by Barry et al. (US 5911710; hereafter Barry).

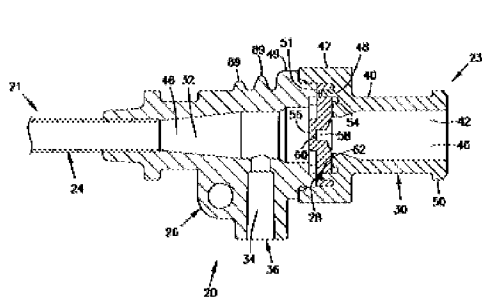


Fig. 2

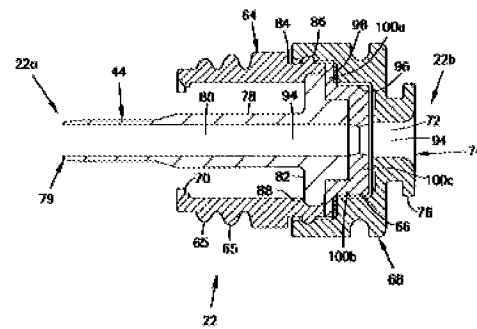


Fig. 3

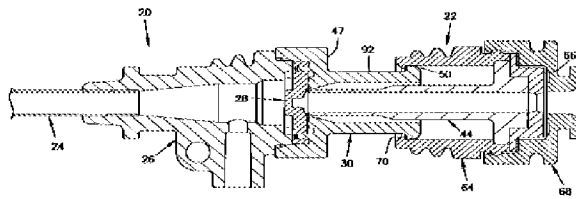


Fig. 1

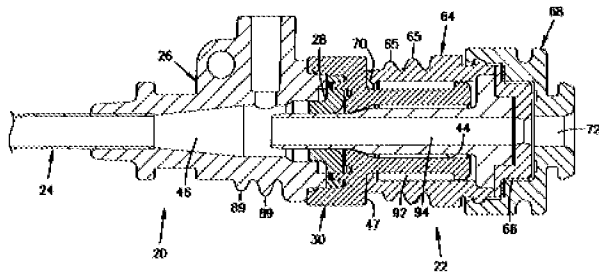


Fig. 4

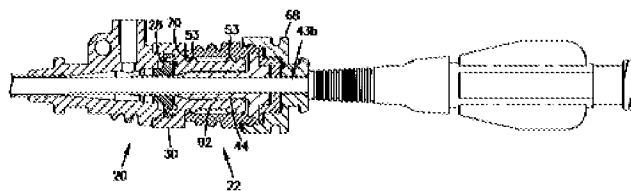


Fig. 7

The cited patent shows in figures 1-4 and 7, the steps of:

- providing a vascular access device having a device lumen and a safety valve on the proximal end thereof (Fig. 2);
- introducing the vascular access device into the body with the distal end of the device lumen being positioned within a vasculature of the body¹;
- attaching a detachable hemostasis valve to the safety valve to open the safety valve (Fig. 1); and
- inserting a device through the hemostasis valve, open safety valve and device lumen (Fig. 7).


Claim Rejections - 35 USC § 103

The following is a quotation of 35 U.S.C. 103(a) which forms the basis for all obviousness rejections set forth in this Office action:

(a) A patent may not be obtained though the invention is not identically disclosed or described as set forth in section 102 of this title, if the differences between the subject matter sought to be patented and the prior art are such that the subject matter as a whole would have been obvious at the time the invention was made to a person having ordinary skill in the art to which said subject matter pertains. Patentability shall not be negated by the manner in which the invention was made.

Claim 3 is rejected under 35 U.S.C. 103(a) as being unpatentable over Barry in view of Melker et al. (US 5,250,038; hereafter Melker). The Barry patent does not disclose a vascular access device having multiple lumens. However, such design would have been considered conventional in the art as evidenced by the teachings of Melker.

¹ In Column 3, lines 62-67, the specification states "[t]he distal end of the sheath tube 24 is adapted for insertion into a patient's artery (not shown). Thus, when sheath tube 24 is inserted into an artery of a patient, fluid communication is established between a patient's bloodstream and the interior passageway 32 of the sheath hub 26".

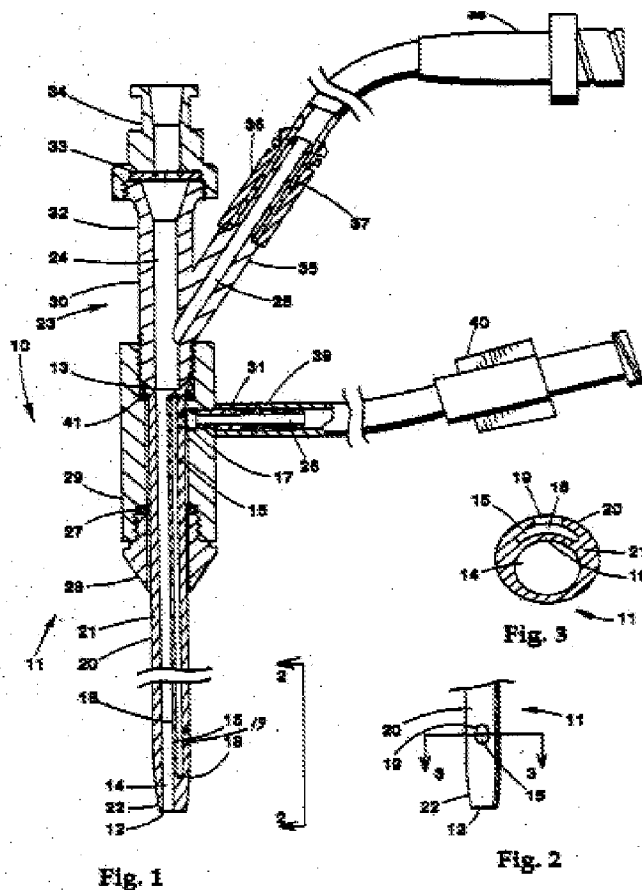

The Melker patent shows in figure 1, a multiple lumen vascular introducer sheath (29). Based on the teachings of the Melker patent, for a person of ordinary skill in the art, modifying the vascular access device disclosed by Barry, with a vascular access device having multiple infusion lumens, as taught by Melker, would have been considered obvious in view of the proven conventionality of this particular cannula design, and moreover, because such modification would have improved the capabilities of the access device by permitting simultaneous insertion of medical instruments into the body and infusion of fluids.

Any inquiry concerning this communication or earlier communications from the examiner should be directed to Manuel A. Mendez whose telephone number is 571-272-4962. The examiner can normally be reached on 0730-1800 hrs.

If attempts to reach the examiner by telephone are unsuccessful, the examiner's supervisor, Mr. Nicholas D. Lucchesi can be reached on 571-272-4977. The fax phone number for the organization where this application or proceeding is assigned is 571-273-8300.

Information regarding the status of an application may be obtained from the Patent Application Information Retrieval (PAIR) system. Status information for published applications may be obtained from either Private PAIR or Public PAIR. Status information for unpublished applications is available through Private PAIR only. For more information about the PAIR system, see <http://pair-direct.uspto.gov>. Should you have questions on access to the Private PAIR system, contact the Electronic Business Center (EBC) at 866-217-9197 (toll-free). If you would like assistance from a USPTO Customer Service Representative or access to the automated information system, call 800-786-9199 (IN USA OR CANADA) or 571-272-1000.

/Manuel A. Mendez/

Primary Examiner, Art Unit 3763

Manuel A. Mendez
Primary Examiner
Art Unit 3763

Application/Control Number: 10/614,549
Art Unit: 3763

Page 7